

## cFluor<sup>®</sup> R685 Anti-Human CD56 (TULY56)

PRODUCT DETAILS	
<b>Catalog Number:</b>	R7-20343 (100 tests) R7-20344 (25 tests)
<b>Reactivity:</b>	Human
<b>Clone:</b>	TULY56
<b>Format:</b>	cFluor <sup>®</sup> R685*
<b>Isotype:</b>	Mouse IgG1.k
<b>Test Dilution:</b>	5 µL / test
<b>Application:</b>	Flow cytometry
<b>Formulation:</b>	Phosphate-buffered saline, pH 7.2, containing 0.09% sodium azide and 0.2% BSA (BSA Country of Origin USA)
<b>Storage:</b>	2-8°C and protected from light. <b>Do not freeze</b>

### PRODUCT DESCRIPTION

The TULY56 monoclonal antibody binds to human CD56, a 120 to 180-kDa type I transmembrane glycoprotein in the immunoglobulin superfamily. Depending on the cytoplasmic domain, CD56 exists in three main isoforms: NCAM-120, NCAM-140, and NCAM-180<sup>1</sup>. CD56, also known as NCAM (Neural Cell Adhesion Molecule), Leu-19 and NKH1, is present on NK and NKT cells. CD56 is also expressed in the brain (cerebellum and cortex) and at neuromuscular junctions. Aberrant CD56 expression is observed in a range of hematological malignancies such as multiple myeloma and leukemia<sup>2</sup> as well as in solid tumors such as lung cancer, ovarian cancer, and neuroblastoma<sup>3</sup>. The antibody was conjugated to a fluorophore and purified by chromatography.


### RECOMMENDED USAGE

Each lot of this antibody is quality control tested using flow cytometric analysis. For flow cytometric staining, the suggested use of this reagent is 5 µL per 1 million cells in a staining volume of 100 µL. If whole blood is analyzed, then use 5 µL per 100 µL. It is recommended that users titrate the antibody to obtain the optimal result for their specific application.


Please briefly centrifuge the reagent vial before use.

Use appropriate personal protective equipment per the product safety data sheet when using this product.

### PRODUCT DATA

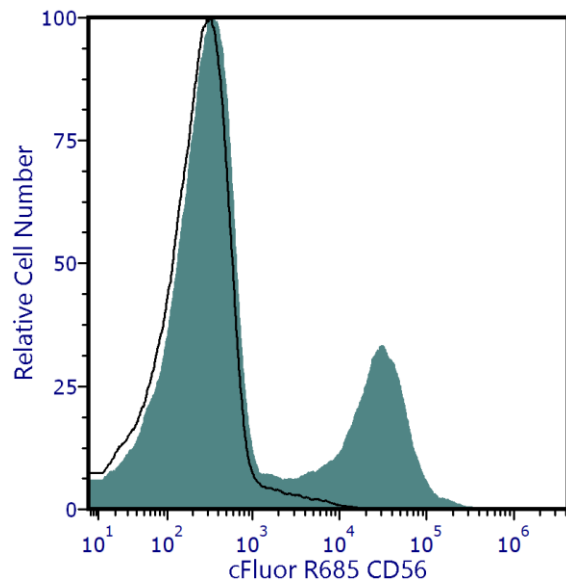

Human peripheral blood was stained with cFluor® R685 CD56 (clone TULY56) (filled histogram) or mouse cFluor® R685 IgG1 isotype control (open histogram). Data shown is gated on lymphocytes.

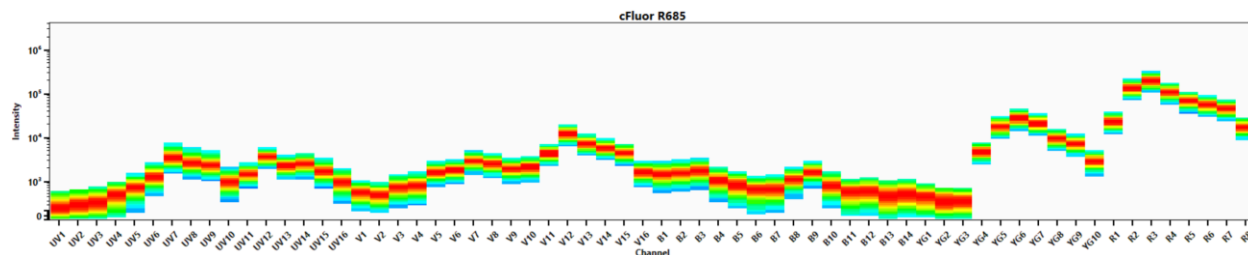

Spectral signature of cFluor® R685 from a Cytek® Aurora 5 laser system equipped with 355, 405, 488, 561 and 640 nm lasers using CytekAssaySetting.

### REFERENCES

1. Van Acker HH, et al. 2017. Front Immunol. 8:892
2. Crossland DL, et al. 2018. Oncogene. 37(27):3686-3697
3. Seidenfaden R, et al. 2006. Neurochem Int. 49(1):1-11

**For Research Use Only. Not intended for use in diagnostic procedures.**

\*cFluor® R685 is equivalent to CF®660C manufactured and provided by Biotium, Inc. under an Agreement between Biotium and Cytek (LICENSEE). The manufacture, use, sale, offer for sale, or import of the product is covered by one or more of the patents or pending applications owned or licensed by Biotium. The purchase of this product includes a limited, non-transferable immunity from suit under the foregoing patent claims for using only this amount of product for the purchaser's own internal research. No right under any other patent claim, no right to perform any patented method, and no right to perform commercial services of any kind, including without limitation reporting the results of purchaser's activities for a fee or other commercial consideration, is conveyed expressly, by implication, or by estoppel.