

cFluor® V420 Anti-Human CD3 (SK7)

PRODUCT DETAILS	
Catalog Number:	R7-20053 (100 tests) R7-20054 (25 tests)
Reactivity:	Human, Chimpanzee
Clone:	SK7
Format:	cFluor® V420
Isotype:	Mouse IgG1, κ
Volume Per Test:	5 µL / test
Application:	Flow cytometry
Formulation:	Phosphate-buffered saline, pH 7.2, containing 0.09% sodium azide and 0.2% BSA (BSA Country of Origin USA)
Storage:	2-8°C and protected from light. Do not freeze

PRODUCT DESCRIPTION

The SK7 monoclonal antibody binds to human epsilon chain of the CD3 antigen/T-cell antigen receptor, a 20 to 30-kDa protein complex. This complex contains a CD3γ, a CD3δ, a CD3ζ (CD247), two CD3ε, and a T-cell receptor (αβ or γδ) heterodimer¹. CD3 is found on all mature T cells, NK T cells and thymocytes. It plays a role in recognizing antigen, activating cytotoxic T cell and T helper cell, and signal transduction². The antibody was conjugated to a fluorophore and purified by affinity chromatography.


RECOMMENDED USAGE

Each lot of this antibody is quality control tested using flow cytometric analysis. For flow cytometric staining, the suggested use of this reagent is 5 µL per 1 million cells in a staining volume of 100 µL. If whole blood is analyzed, then use 5 µL per 100 µL. It is recommended that users titrate the antibody to obtain the optimal result for their specific application.


Please briefly centrifuge the reagent vial before use.

Use appropriate personal protective equipment per the product safety data sheet when using this product.

PRODUCT DATA

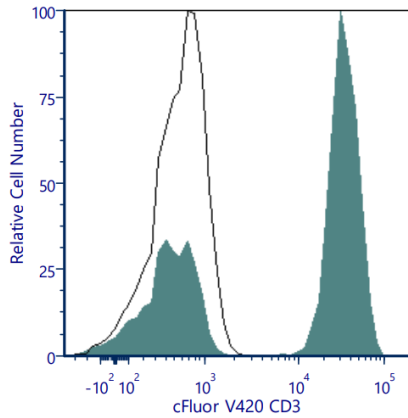

Human peripheral blood was stained with cFluor® V420 CD3 (clone SK7) (filled histogram) or mouse cFluor® V420 IgG1, κ isotype control (open histogram). Data shown is gated on lymphocytes.

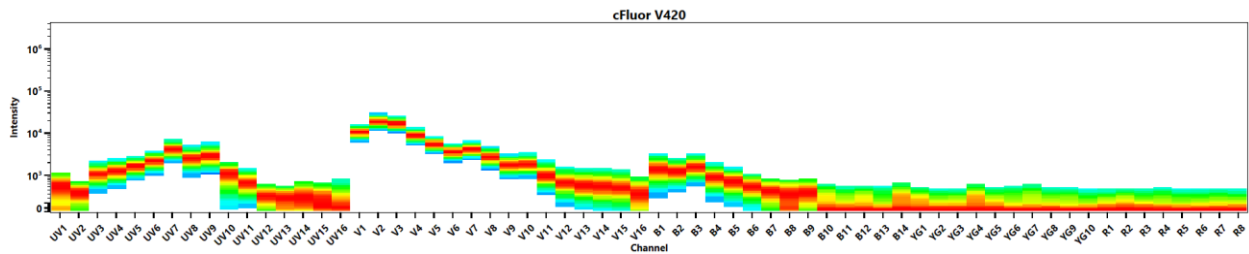

Spectral signature of cFluor® V420 from a Cytek® Aurora 5 laser system equipped with 355, 405, 488, 561 and 640 nm lasers using CytekAssaySetting.

REFERENCES

1. Dong, D., et al. 1981. Nature. 573, 546–552
2. Weiss A, et al. 1991. Semin Immunol. (5):313-24

For Research Use Only. Not intended for use in diagnostic procedures.