

cFluor[®] V450 Anti-Human CD16 (3G8)

PRODUCT DETAILS	
Catalog Number:	R7-20183 (100 tests) R7-20184 (25 tests)
Reactivity:	Human
Clone:	3G8
Format:	cFluor [®] V450
Isotype:	Mouse IgG1, κ
Test Dilution:	5 μ L / test
Application:	Flow cytometry
Formulation:	Phosphate-buffered saline, pH 7.2, containing 0.09% sodium azide and 0.2% BSA (BSA Country of Origin USA)
Storage:	2-8°C and protected from light. Do not freeze

PRODUCT DESCRIPTION

The 3G8 monoclonal antibody binds to IgG receptor III (Fc γ RIII) that are in two forms: CD16a ((Fc γ RIIIA) and CD16b ((Fc γ RIIIB). With 95% sequence similarity, they are a conventional 50-65 kD polypeptide-anchored transmembrane protein and a 48 kD GPI-anchored protein, respectively. CD16a is expressed on NK cells and macrophages while CD16b is expressed on neutrophils ⁽¹⁾⁽²⁾. CD16a also plays a crucial role for antibody-dependent cellular cytotoxicity (ADCC) by NK cells ⁽³⁾. The antibody was conjugated to a fluorophore and purified by affinity chromatography.


RECOMMENDED USAGE

Each lot of this antibody is quality control tested using flow cytometric analysis. For flow cytometric staining, the suggested use of this reagent is 5 μ L per 1 million cells in a staining volume of 100 μ L. If whole blood is analyzed, then use 5 μ L per 100 μ L. It is recommended that users titrate the antibody to obtain the optimal result for their specific application.

Please briefly centrifuge the reagent vial before use.


Use appropriate personal protective equipment per the product safety data sheet when using this product.

PRODUCT DATA

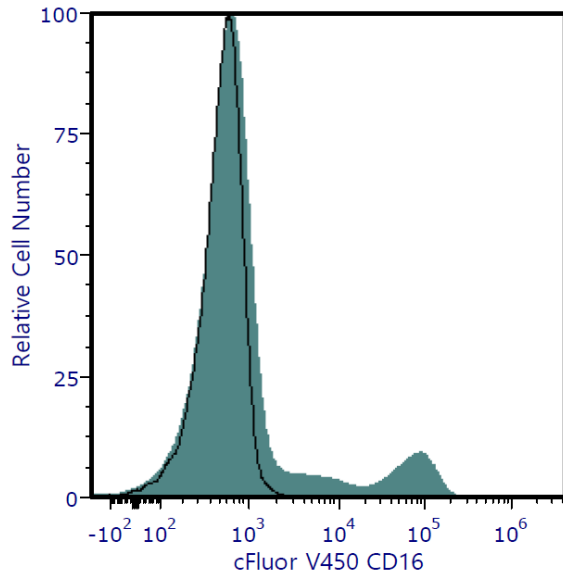

Human peripheral blood stained with cFluor® V450 CD16 (clone 3G8) (filled histogram) or mouse cFluor® V450 IgG1, κ isotype control (open histogram). Data shown is gated on Lymphocytes.

Spectral signature of cFluor® V450 from a Cytex® Aurora 5 laser system equipped with 355, 405, 488, 561 and 640 nm lasers using CytexAssaySetting.

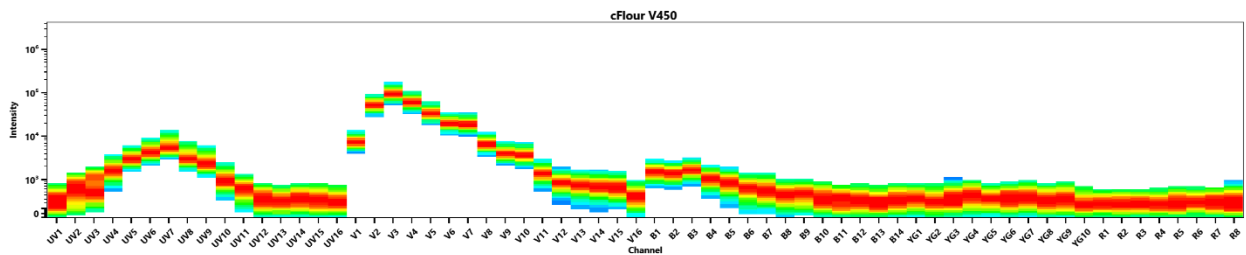

REFERENCES

1. Wirthmueller U, et al. 1992. J Exp Med. 175:1381
2. Smed-Sørensen A, et al. 2008. Blood. 111:5037
3. Wei H Y, et al, 2016. Sci Rep. 6:34310

For Research Use Only. Not intended for use in diagnostic procedures.